Installation / Operation Instructions

M9/M11 Service Diagnostics

REQUIRED TOOLS

- Interface Cable, (RS232 to TTL) part number 015-1751-00.
- RS232 Cable, 6 ft. length with one each DB9 Male and Female connectors. *Do **not** use a **Null** Modem cable.* Use Radio Shack Part # 26-117 or equivalent.
- Documark CD Version 8.0 or above.
- Computer with CD drive (Desk PC or Laptop).

INSTALLATION

WARNING.

Unplug Sterilizer before removing any covers or beginning installation. When sterilizer is plugged in during Diagnostics power is present. Use caution to prevent personal injury.

A. Remove right side cover.

B. Connect interface cable to RS232 (J10) plug connector on sterilizer PC control board.

NOTE

When making connections to computer note the port (A,B, etc.) that the RS232 is connected in.

C. Connect RS232 Cable to interface cable and the other end to RS232 plug connector on back of PC or laptop computer.

D. Boot up computer and insert Documark, version 8.0 or above into CD drive.

E. After opening M9 / M11 Diagnostics, plug Sterilizer into an outlet.

NOTE

Follow the steps in the Sterilizer Diagnostics. For repair or adjustment procedures refer to Sterilizer Service and Parts.

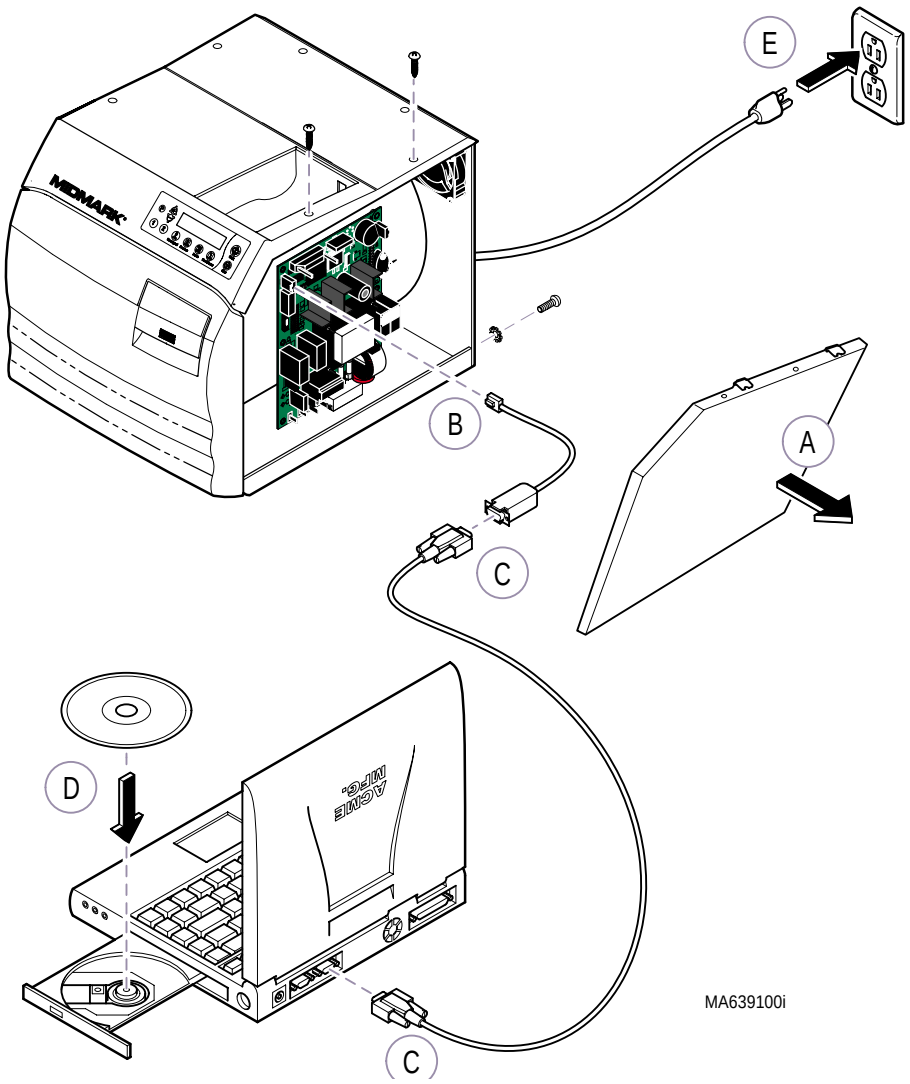

© Midmark Corporation - 2001